

SUMMARY TEST DATA ON DTA-0R5G18G-60-CD-1

Customer: _____
 SO No: _____
 Model No: DTA-0R5G18G-60-CD-1
 Serial No: 13384
 Part No: _____

Tested By: K. Mansfield
 Date: 11/23/2021
 Drawing No: 27617783 Rev: A1

TEST. ITEM NO	PARAMETERS	SPECIFIED VALUE	TEST RESULTS	QA QC	
1	Frequency Range:	0.5 GHz – 18 GHz	0.5 GHz – 18 GHz	PMI QA 2	
2	Insertion Loss:	4.8 dB Max.	4.1 dB See Plot		
3	VSWR:	2.0:1 Max.	1.83:1 See Plot		
4	Flatness to 20 dB:	± 1.0 dB Typ.	0.54 dB See Plot		
6	Flatness to 40 dB:	± 1.25 dB Typ.	0.65 dB See Plot		
7	Flatness to 60 dB:	± 3.0 dB Typ.	1.85 dB See Plot		
8	Accuracy of Attenuation 0 to 20 dB:	± 1.0 dB Typ.	0.09 dB See Plot		
9	Accuracy of Attenuation 20 to 40 dB:	± 1.5 dB Typ.	0.11 dB See Plot		
10	Accuracy of Attenuation 40 to 60 dB:	± 2.0 dB Typ.	0.13 dB See Plot		
11	Switching Speed:	1.0 us Max.	< 1.0 us See Typical Characteristics		
12	DC Supply:	+15VDC @ 155 mA	110 mA		PMI QA 2

Programed Attenuation	Attenuation	Accuracy of Attenuation	Flatness dB
dB	dB	dB	±dB
0.0625	0.05	0.01	0.01
0.125	0.11	0.01	0.01
0.25	0.24	0.01	0.02
0.50	0.48	0.02	0.04
1.00	0.98	0.02	0.10
2.00	1.98	0.02	0.14
4.00	3.97	0.03	0.22
8.00	7.96	0.04	0.37
16.00	15.92	0.06	0.49
32.00	31.94	0.06	0.62
62.00	62.15	-0.15	2.11
63.94	64.07	-0.14	2.30

Programed Attenuation	Attenuation	Accuracy of Attenuation	Flatness dB
dB	dB	dB	±dB
5.00	4.93	0.07	0.26
10.00	9.97	0.03	0.43
15.00	14.91	0.09	0.47
20.00	19.93	0.07	0.54
25.00	24.89	0.11	0.53
30.00	29.94	0.06	0.59
35.00	34.94	0.06	0.62
40.00	39.96	0.04	0.65
45.00	44.99	0.01	0.97
50.00	50.04	-0.04	1.06
55.00	55.05	-0.05	1.44
60.00	60.13	-0.13	1.85

QA/QC Approval: _____





PMI
QA 2

Date: _____

11/24/2021


SUMMARY TEST DATA ON DTA-0R5G18G-60-CD-1

13384

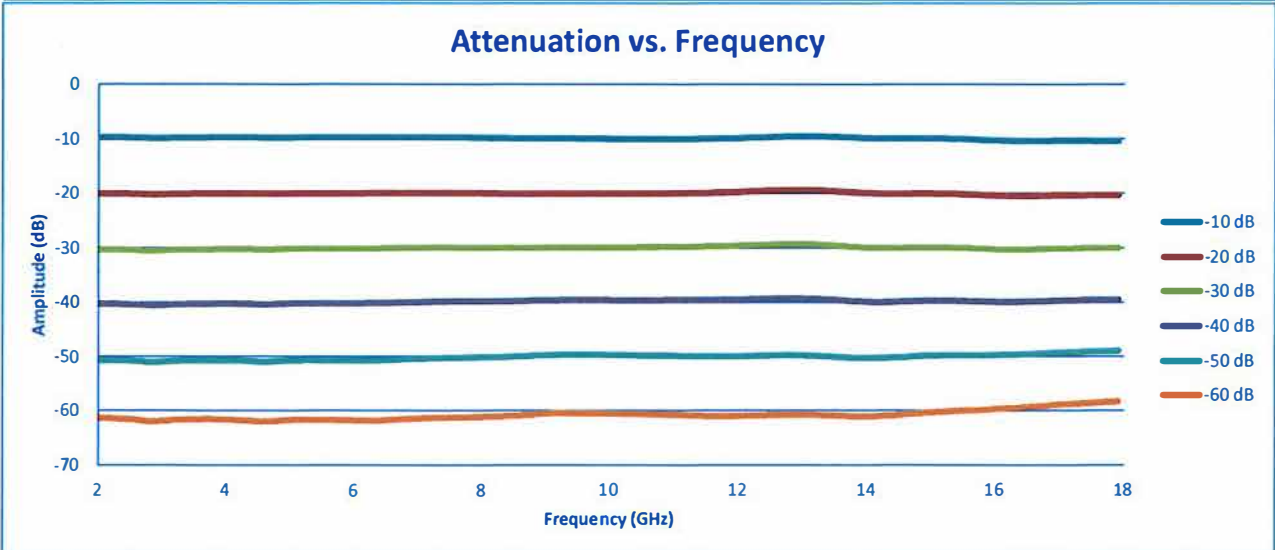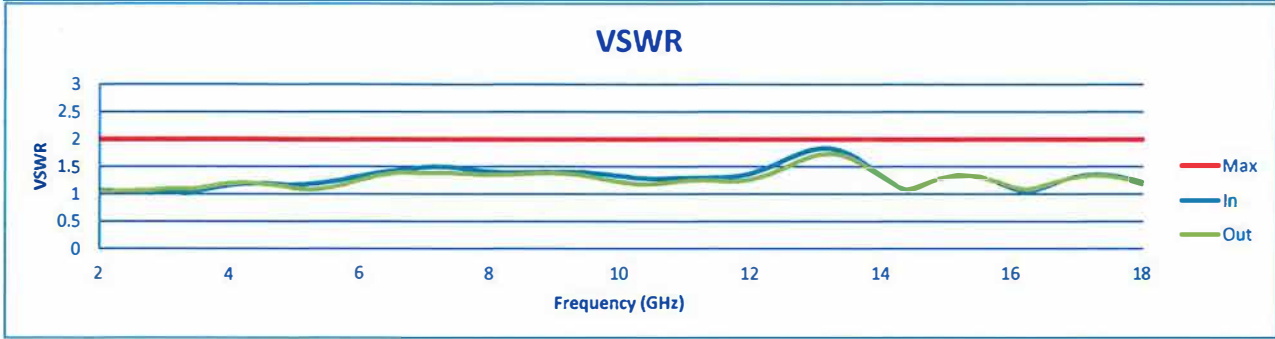

7311-F Grove Road Frederick, MD 21704 USA Phone: (301)662-5019 Fax: (301)662-1731
Email: sales@pmi-rf.com

**SUMMARY TEST DATA
ON
DTA-0R5G18G-60-CD-1**

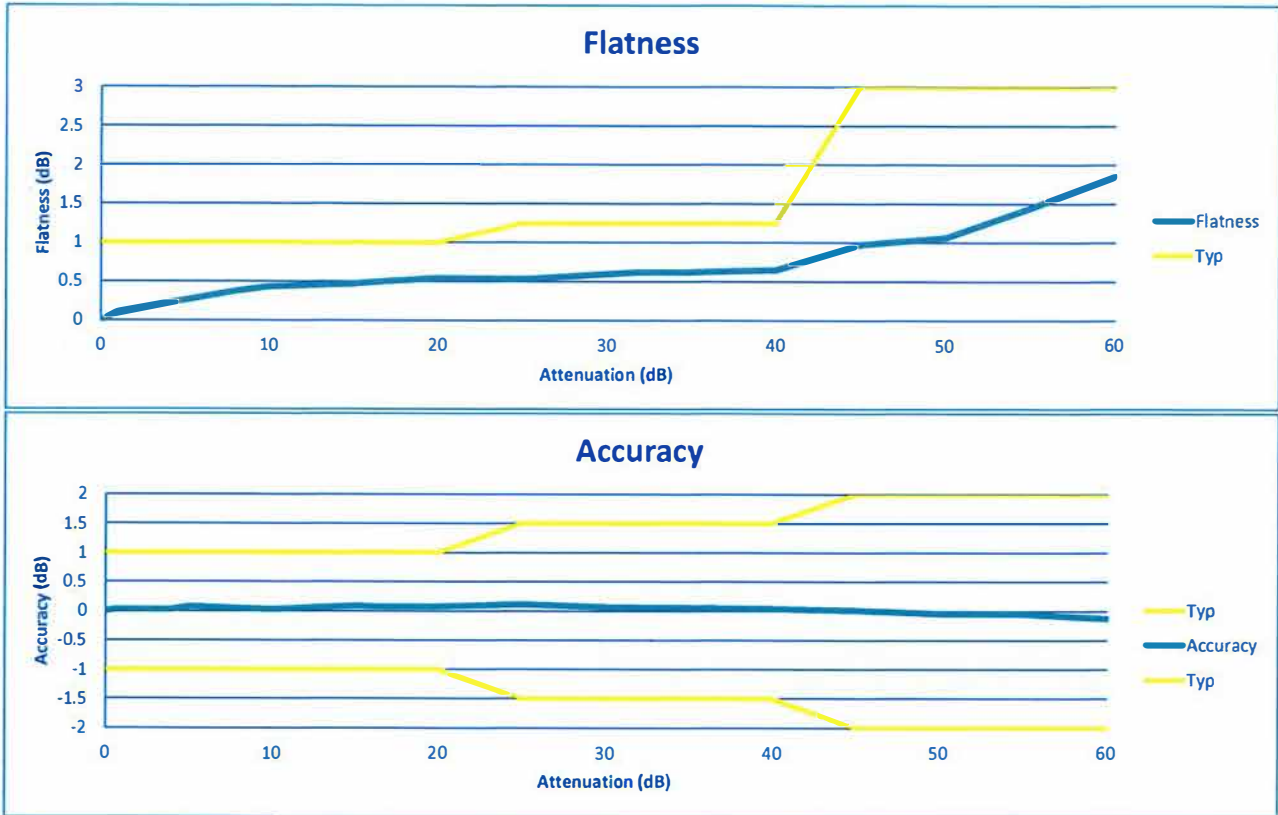

7311-F Grove Road Frederick, MD 21704 USA Phone: (301)662-5019 Fax: (301)662-1731
Email: sales@pmi-rf.com